


E•LUMINEXX™

VASCULAR & BILIARY STENT




Designed for Endurance and Delivering
VISIBLE RESULTS

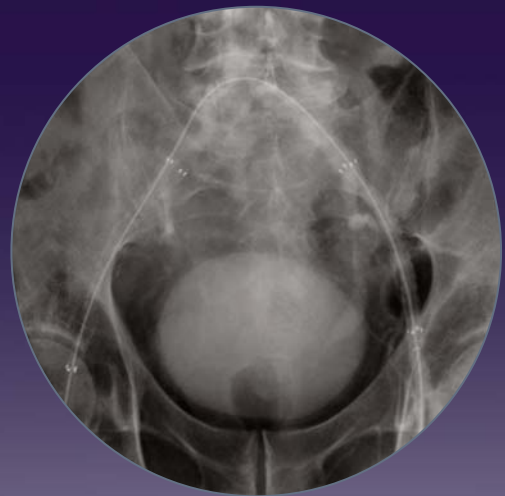

BARD
**PERIPHERAL
VASCULAR**

LABORATORY TEST OUTCOMES

Comparative Stent Fatigue Survival Rates Axial Compression & Compression / Elongation Tests

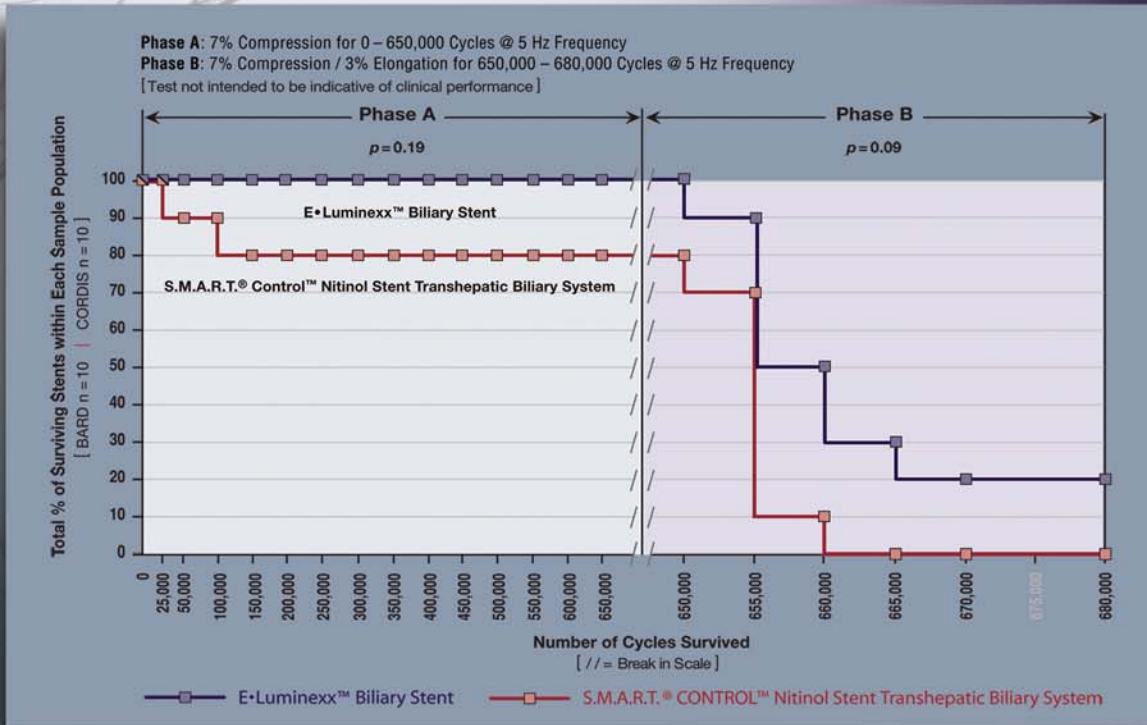


Biliary Stent Surface Finish Comparison

SEM

Scanning Electron Microscopy

Bard Peripheral Vascular, Inc.

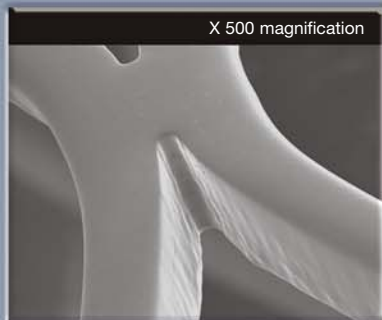

BARD® E•LUMINEXX™
BILIARY STENT

Cordis Corporation



S.M.A.R.T.® CONTROL™
NITINOL STENT TRANSHEPATIC
BILIARY SYSTEM

Boston Scientific Corporation



SENTINOL™
SELF-EXPANDING NITINOL
BILIARY STENT SYSTEM

The unique, multi-step electro-polishing technology developed by BARD® reduces microscopic burrs and microcracks





CLINICAL TRIAL OUTCOMES


A Review of Clinical Trial Data^{1, 2, 3, 4}

The displayed clinical data are taken from a number of different studies, not a head-to-head study. Each study may have varying patient profiles and protocol structures that may affect the outcome rates set forth below, and therefore is not intended to demonstrate superiority of any one product.

The LUMINEXX® Iliac Clinical Study met the success criteria for the primary endpoint; posterior probability of at least 96% that the 9-month MACE rate was < 25%. MACE included peri-procedural death, TLR and stent segment restenosis and non-study stent. (Non-study stent was added post hoc to the protocol definition of MACE.)

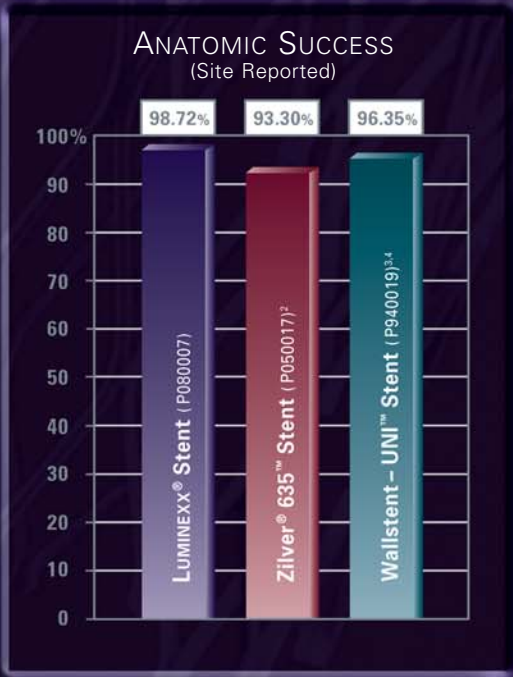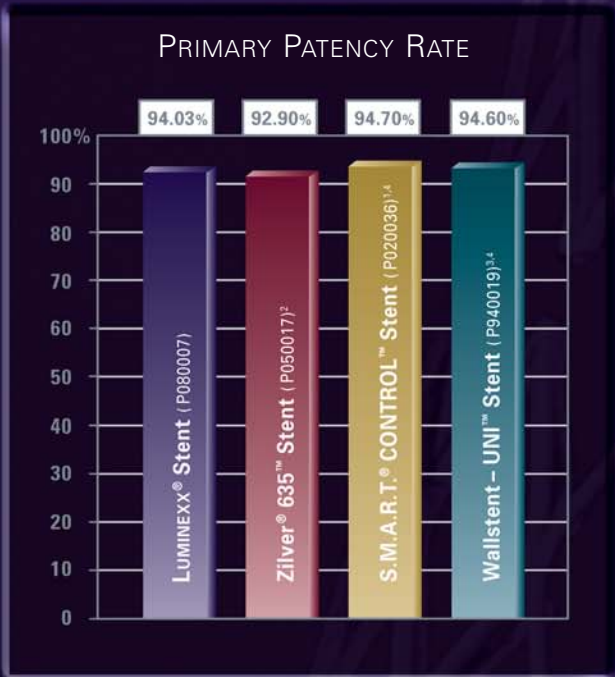

The LUMINEXX® Iliac Clinical Study demonstrated competitive results when considering Primary Patency Rate, Anatomic Success and Mortality Rate.

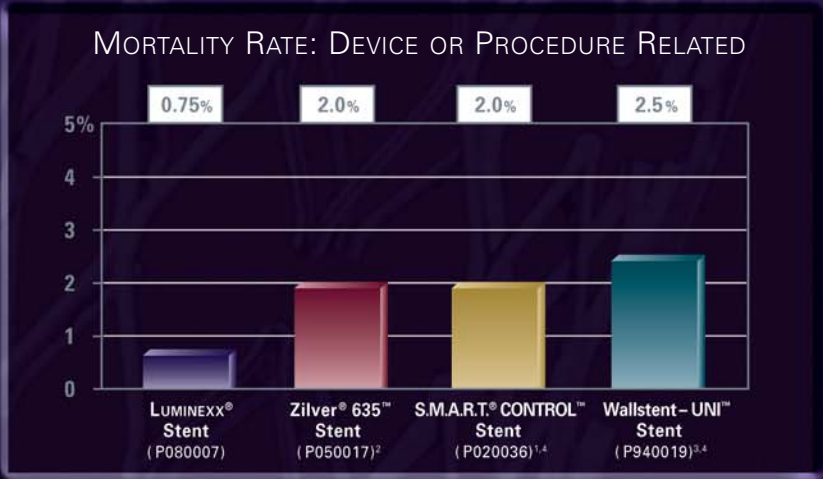

Consult each respective study for more information on how mortality rates were calculated. Mortality rates within a trial may not be predictive of patient outcomes outside of a controlled clinical trial.

E•LUMINEXX™

VASCULAR & BILIARY STENT

With the...

PerforMAXX® Grip

Order Information

Stent Diameter [mm]	Catheter Length [cm]	Stent Length [mm]	Product Code	Stent Diameter [mm]	Catheter Length [cm]	Stent Length [mm]	Product Code
7	80	20	ZBM07020	9	80	20	ZBM09020
		30	ZBM07030			30	ZBM09030
		40	ZBM07040			40	ZBM09040
		60	ZBM07060			60	ZBM09060
		80	ZBM07080			80	ZBM09080
	100	ZBM07100	100		ZBM09100		
	135	20	ZBL07020		135	20	ZBL09020
		30	ZBL07030			30	ZBL09030
		40	ZBL07040			40	ZBL09040
		60	ZBL07060			60	ZBL09060
80		ZBL07080	80	ZBL09080			
100	ZBL07100	100	ZBL09100				
8	80	20	ZBM08020	10	80	20	ZBM10020
		30	ZBM08030			30	ZBM10030
		40	ZBM08040			40	ZBM10040
		60	ZBM08060			60	ZBM10060
		80	ZBM08080			80	ZBM10080
	100	ZBM08100	100		ZBM10100		
	135	20	ZBL08020		135	20	ZBL10020
		30	ZBL08030			30	ZBL10030
		40	ZBL08040			40	ZBL10040
		60	ZBL08060			60	ZBL10060
80		ZBL08080	80	ZBL10080			
100	ZBL08100	100	ZBL10100				

For All Product Codes: 6F Catheter System; 0.035" Guidewire.

6F BARD S.A.F.E.®
Delivery System

PHYSICIAN'S SIGNATURE

For more information, contact:

Bard Peripheral Vascular, Inc.
1625 W. 3rd Street
Tempe, AZ 85281
USA

Tel: 1-480-894-9515

1-800-321-4254

Fax: 1-480-966-7062

1-800-440-5376

www.bardpv.com

1. S.M.A.R.T.® Control™ Nitinol Stent System. Premarket Approval Application Number P020036. Summary of Safety and Effectiveness Data, 2003.
2. Zilver® 635™ Vascular Stent. Premarket Approval Application Number P050017. Summary of Safety and Effectiveness Data, 2006.
3. Wallstent-Uni™ Iliac Endoprosthesis. Premarket Approval Application Number P940019. Summary of Safety and Effectiveness Data, 1996.
4. Ponec D, Jaff MR, Swischuk J, Feiring A, Laird J, Mehra M, Popma JJ, Donohoe D, Firth B, Heim E, Snead D. The nitinol SMART stent vs. Wallstent for suboptimal iliac artery angioplasty: CRISP-US trial results. *J Vasc Interv Radiol.* 2004;15:911-918.

Please consult product labels and package inserts for indications, contraindications, hazards, warnings, cautions, and information for use.

Bard, BARD S.A.F.E., E•LUMINEXX, LUMINEXX and PerforMAXX are trademarks and/or registered trademarks of C. R. Bard, Inc. or an affiliate. All other trademarks are property of their respective owners.

© 2008 C. R. Bard, Inc. All Rights Reserved.

♦ S.A.F.E. = Secure Adhesive Free Tip Design.

S11683 Rev. 0



BARD

PERIPHERAL
VASCULAR