


Woven Vascular Prosthesis

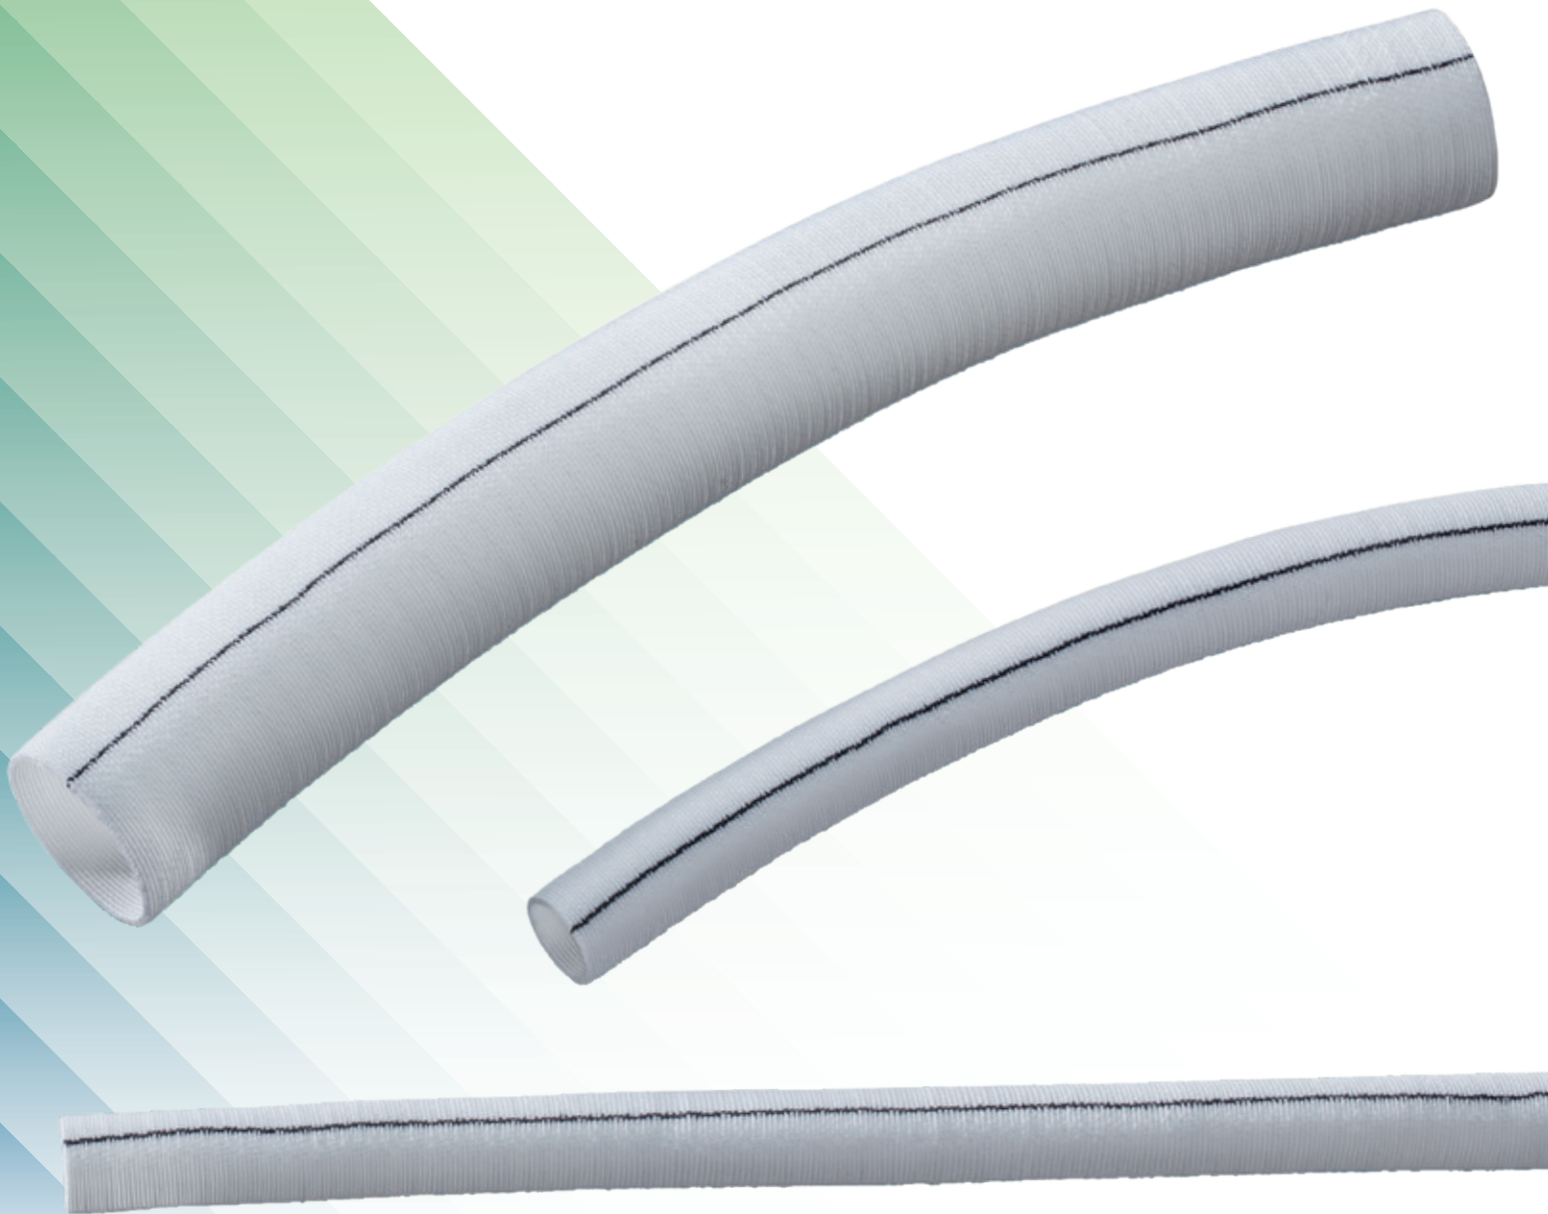

FlowWeave Bioseal

- Specific weaving techniques for high burst resistance and low dilatation^{1,2}
- Different internal and external surface structures enable blood flow optimization
- Aldehyde and isocyanate free Bioseal impregnation using dehydrothermal crosslinked collagen guarantees primary sealing of the blood in the prosthesis³
- Concentric crimping and the guide line allow precise positioning of the prosthesis
- Soft and supple texture for easy handling

ORDERING INFORMATION

Catalogue No.	Ø (mm)	Length (cm)
45ST1508	8	15
45ST3008	8	30
45ST1510	10	15
45ST3010	10	30
45ST1512	12	15
45ST3012	12	30
45ST1520	20	15
45ST3020	20	30
45ST1522	22	15
45ST3022	22	30
45ST1524	24	15
45ST3024	24	30
45ST1526	26	15

Catalogue No.	Ø (mm)	Length (cm)
45ST3026	26	30
45ST1528	28	15
45ST3028	28	30
45ST1530	30	15
45ST3030	30	30
45ST1532	32	15
45ST3032	32	30
45ST1534	34	15
45ST3034	34	30



ARTIVION™

Learn more at [artivion.com](https://www.artivion.com)

References:

- 1 JOTEC GmbH, subsidiary of CryoLife, Inc.: Internal mechanical test data
- 2 Bell C-M.: [Study on the issue of expansion of textile implants] – (internal data, JOTEC GmbH)
- 3 Freischlag J, J.A. and Moore, W. S.: Clinical Experience with a Collagen-Impregnated Knitted Dacron Vascular Graft; Ann of Vascular Surg 1990; 4(5): 449-454

Indications: FlowWeave Bioseal is indicated in arterial aneurysms and vascular occlusions. The primary indication for FlowWeave Bioseal is vascular replacement in the thoracic and abdominal aortas, although it can also be used in peripheral vascular applications involving vessel diameters of at least 6 mm.

All products and indications are not available/approved in all markets. All trademarks are owned by Artivion, Inc. or its subsidiaries. On-X Life Technologies, Inc. Jotec GmbH and Ascyrus Medical GmbH are wholly owned subsidiaries of Artivion, Inc. © 2022 Artivion, Inc. All rights reserved.


Artivion, Inc.

1655 Roberts Blvd., NW
Kennesaw, GA 30144 USA
Phone: +1-888-427-9654
Fax: +770-590-3753
E-mail: inquiries@artivion.com
For contact information by region, please visit www.artivion.com/contact

JOTEC GmbH, Lotzenäcker 23, 72379 Hechingen, Germany

JT-BR-0450200-EN V03 11/2022

Knitted Vascular Prosthesis

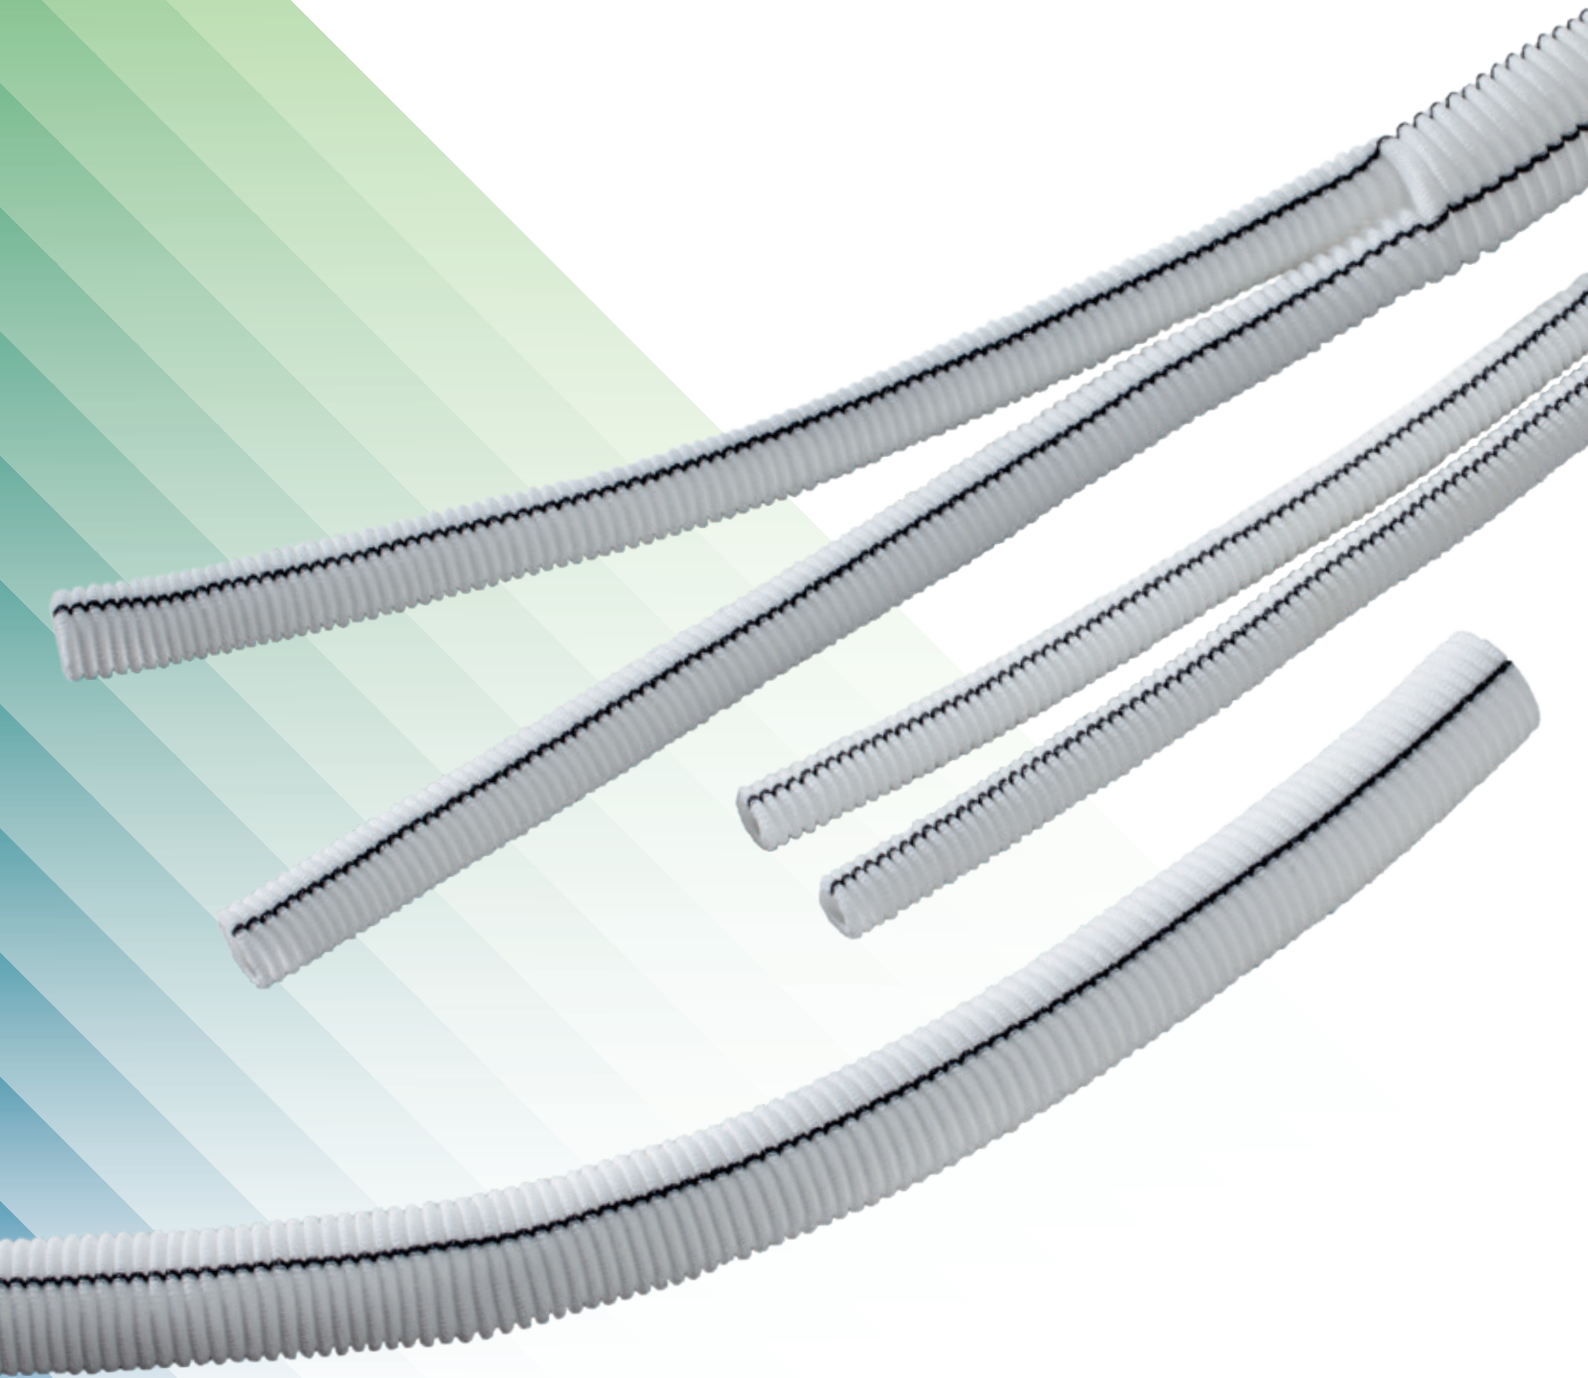

FlowNit Bioseal

Knitted vascular prostheses:

- Specific knitting techniques for high burst resistance and low dilatation¹²
- Aldehyde and isocyanate free BIOSEAL impregnation using dehydrothermal crosslinked collagen guarantees primary sealing of the blood in the prosthesis³
- Concentric crimping and the guide line allow precise positioning of the prosthesis
- Soft and supple texture for easy handling

Ordering Information

Straight prostheses



Catalogue No.	Ø (mm)	Length (cm)
35ST1506	6	15
35ST3006	6	30
35ST6006	6	60
35ST1507	7	15
35ST3007	7	30
35ST6007	7	60
35ST1508	8	15
35ST3008	8	30
35ST6008	8	60
35ST0008	8	100
35ST1510	10	15
35ST3010	10	30
35ST6010	10	60
35ST0010	10	100

Straight prostheses

Catalogue No.	Ø (mm)	Length (cm)
35ST1512	12	15
35ST3012	12	30
35ST1514	14	15
35ST3014	14	30
35ST1516	16	15
35ST3016	16	30
35ST1518	18	15
35ST3018	18	30
35ST1520	20	15
35ST3020	20	30
35ST1522	22	15
35ST3022	22	30
35ST1524	24	15
35ST3024	24	30

Bifurcated prostheses

Catalogue No.	Ø (mm)	Length (cm)
35BI1206	12x6	45
35BI1407	14x7	45
35BI1608	16x8	45
35BI1809	18x9	45
35BI2010	20x10	45
35BI2211	22x11	45
35BI2412	24x12	45



ARTIVION™

Learn more at artivion.com

References:

- 1 JOTEC GmbH, subsidiary of CryoLife, Inc.: Internal mechanical test data
- 2 Bell C-M.: [Study on the issue of expansion of textile implants] – (internal data, JOTEC GmbH)
- 3 Freischlag J, J.A. and Moore, W. S.: Clinical Experience with a Collagen-Impregnated Knitted Dacron Vascular Graft; Ann of Vascular Surg 1990; 4(5): 449-454

Indications: FlowNit Bioseal is indicated in arterial aneurysms and vascular occlusions. FlowNit BIOSEAL is primarily indicated for vascular replacement in the entire abdominal aorta and in peripheral vascular applications involving vessel diameters of at least 6 mm.

All products and indications are not available/approved in all markets. All trademarks are owned by Artivion, Inc. or its subsidiaries. On-X Life Technologies, Inc. Jotec GmbH and Ascyrus Medical GmbH are wholly owned subsidiaries of Artivion, Inc. © 2022 Artivion, Inc. All rights reserved.

Artivion, Inc.
 1655 Roberts Blvd., NW
 Kennesaw, GA 30144 USA
 Phone: +1-888-427-9654
 Fax: +770-590-3753
 E-mail: inquiries@artivion.com
 For contact information by region, please visit. www.artivion.com/contact

 JOTEC GmbH, Lotzenäcker 23, 72379 Hechingen, Germany

JT-BR-0350200-EN V03 11/2022